



# JAMMU AND KASHMIR MEDICAL SUPPLIES CORPORATION LTD.

(Public Sector Undertaking of the Government of Jammu and Kashmir)

Corporate Head Office: Corporate Head Office: Plot No. 58, Friends Colony Satyam Road Trikuta Nagar Jammu

Corporate Office: Corporate Office Kashmir: Near Haj House, Bemina(190018), Srinagar

email: [jkmscljepm@gmail.com](mailto:jkmscljepm@gmail.com); website: [www.jkmscl.nic.in](http://www.jkmscl.nic.in)

JKMSCL

M/s Siddidhata Associates  
Jammu (Bidder)

No: JKMSCL/2024/6330-42

Dated: 23/10-2024.

**Sub: E.bid for the finalization of Rate Contract for the procurement of "Machinery & Equipments" - issuance of rate contract thereof.**

Ref No.

1. NIT No. JKMSCL/Mach/2023/574 dated 03.02.2023

2. Minutes of Purchase Committee vide No. JKMSCL /MD/2023-24/1701-11 Dated 19.01.2024

3. LOI issued vide No. JKMSCL/2024/1388-91 dated 22.05.2024.

Dear Sir,

As per the decision of the Purchase Committee, the Jammu and Kashmir Medical Supplies Corporation J&K has approved the following item/item(s) under group "Machinery & Equipments" in your favour on the quoted rates by you in the NIT:

S. No.	Name of Item	currency	Basic Rate without Tax with Conversion (1)	Taxes (2)	Total Amount (in Rs) with taxes (1+2)
1.	<b>Hemo Dialysis Machine</b> M/s Nipro Medical (India) Pvt Ltd, Chennai, India (Importer)  M/s Nipro Medical Pvt Ltd, Japan (Manufacturer)  Model: Surdial 55 Plus	INR	750000.00	90000.00	840000.00  (Rupees eight lakh forty thousand only)

The approved rates for Comprehensive Maintenance Contract after the expiry of warranty period of 05 (Five) years are as follows:

S.No	Name of Item	CMC for five years
1	<b>Hemo Dialysis Machine</b>	6 <sup>th</sup> yr = 41500.00 7 <sup>th</sup> yr = 41500.00 8 <sup>th</sup> yr = 41500.00 9 <sup>th</sup> yr = 47200.00 10 <sup>th</sup> yr = 47200.00
		Total CMC amount 218900.00

### Terms and Conditions:

- Delivery Site :** Rate are FOR Drug warehouse of JKMSCL/any Govt. Institution of J&K State, wherever Installation is required.
- Validity :** The rate contract shall remain valid for a period of two years from the date of issuance of the Contract which may be extended for a period of 90 days or till such time the new rate contract is finalized, whichever is earlier, with mutual consent of JKMSCL and successful bidder.
- Taxes:** As mentioned above and as applicable.
- Warranty:** Five Years from the date of installation.
- Performance Security**  
You are further required to deposit the performance security equivalent to 5% of the total invoice value in the shape of Bank Guarantee in favour of FA/CAO, JKMSCL within seven days from the date of issuance of Purchase Order(s) from time to time.
- Supplies**  
Within 90 days from the date of issuance of supply order.
- Penalty**  
In case In case of extension in the delivery period with liquidated damages, recovery of liquidated damages shall be made at the rate of 0.25% per day for every day of delay subject to maximum of 10%.

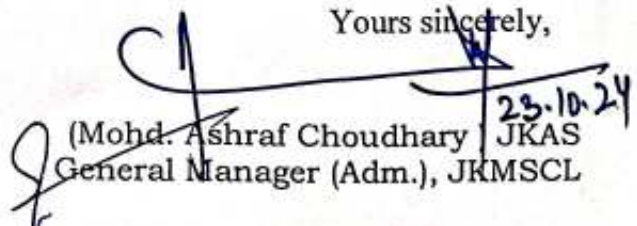


8. **Installation:** Installation / commissioning and necessary training for upkeep of the equipment shall be provided free of cost.
9. **Availability of Spares:** Firm shall certify that the parts of the equipment shall remain available at least for a period of **five years** after the year of expiry of warranty period of five years.
10. You have to certify that the rates mentioned above as quoted by your firm are the lowest rates applicable to all Govt./private Institution/PSU etc. Variation found if any, during the rate contract period by the Corporation/Intending department or any other agency shall be the sole responsibility of the Contractor/Supplier/manufacturer/importer.
11. The supplier/manufacturer/importer shall ensure to supply the Brand new and unused item(s) strictly as per specifications/sample(s) approved. Variations found, if any, in instant case/or in later stages by the Corporation/Intending department/any other agency which may lead to sub standard or Not of standard/approved quality, shall be the sole responsibility of the supplier/ manufacturer/ importer/contractor.
12. JKMSCL is at liberty to get the feedback from the end-user department/intending department regarding the functioning of the machinery & equipment supplied by your agency. Adverse report, if any, may lead to strict action against you under rules/terms & conditions of the NIT/guidelines issued by the Govt. from time to time.
13. **Fall Clause:** The prices under contract shall be subject to price fall clause. The prices charged for the goods supplies under the contract by successful bidder shall in no event exceed the lowest price at which the successful bidder sells the goods or offers to sell the goods of identical description to any other person(s)/Organization(s) including procurement agencies or any other department of Central Govt. or State Govt. as the case may be during the period till the performance of the contract. If at any time, during the period of the contract, the bidder reduces the sales price chargeable under the contract, he shall forth with notify such reduction to the JKMSCL, J&K and the price payable under the contract for the stores supplied after the date of coming into force of such reduction or sale shall stand reduced correspondingly. It imply that if the contract holder quotes/ reduces its price to render similar goods at a price lower than the contract price to anyone in the Central/State Govt. at any time during the currency of contract including extension period, the contract price shall be automatically be reduced with effect from the date of reducing or quoting lower price for all delivery of subject matter of procurement under contract and the contract shall be amended accordingly.
14. **Risk Purchase :** If the bidder is unable to complete the supply within the specified or extended period, the corporation shall be entitled to purchase the goods or any part thereof from elsewhere without notice to the bidder on his (i.e., bidders) account at his cost and risk, with the prior approval of Managing Director JKMSCL, J&K. The bidder shall be liable to pay any loss or damage which the purchasing officer may sustain by reasons of such failure on the part of the bidder.  
The bidder shall not be entitled to any gain on such purchases made against default. The recovery of such loss or damage shall be made from any sums accruing to the bidder under this or any other contract with the corporation/government. If recovery is not possible from the bill and the bidder fails to pay the loss or damage within one month of the demand, the recovery of such amount or sum due from the bidder shall be made from the bidder. In case supplier fails to deliver ordered goods, the risk purchases may be made at market rate from any other firm. It is mandatory for the approved supplier to acknowledge receipt of orders within seven days from the date of dispatch of order, failing which the procuring entity will be at liberty to initiate action to purchase the items on risk purchase provision at the expiry of the prescribed supply period.
15. **Orders shall only be placed on the basis of actual requirement and funds as available under the relevant Head of Accounts.**
16. **Payment shall be released after the execution of the agreement.**
17. **Approved technical specifications shall remain same as per NIT (Annexure I)**

All the terms and conditions of the NIT, Standard Procurement of Procedure (SPP) of JKMSCL & LOI shall be part of this Rate Contract.


*Issued with the decision and authorization of Purchase Committee of JKMSCL vide its minutes No. JKMSCL /MD/2023-24/1701-11 Dated 19.01.2024.*

Yours sincerely,

  
(Mohd. Ashraf Choudhary) JKAS  
General Manager (Adm.), JKMSCL  
23-10-24

**Copy for information to the:-**

1. Principal, Govt. Medical College, Srinagar (Kashmir) (Director, Board of Directors- JKMSCL).
2. Principal, Government Medical College, Jammu (Director, Board of Directors JKMSCL).
3. Principal, Government Dental College, Srinagar (Director, Board of Directors- JKMSCL).

4. Principal, Government Dental College, Jammu (Director, Board of Directors- JKMSCL).
  5. Director General, Indian System of Medicines, J&K (Director, Board of Directors- JKMSCL).
  6. Director, Family Welfare, MCH & Immunization, J&K (Director, Board of Directors- JKMSCL).
  7. Director, Health Services, Jammu (Director, Board of Directors- JKMSCL).
  8. Director, Health Services, Kashmir (Director, Board of Directors- JKMSCL).
  9. Mission Director, NHM, J&K (Director, Board of Directors- JKMSCL).
  10. Controller, Drug & Food Control Organization, J&K (Director, Board of Directors JKMSCL).
  11. F.A/Chief Accounts Officer, J&K Medical Supplies Corporation Limited.
  12. General Manager – (P&S), J&K Medical Supplies Corporation Limited.
- 



<b>Specification for Hemodialysis Machine</b>	
1	The Machine should be of latest technology with microprocessor controlled.
2	Machine should have at least 10" colour TFT display operated by soft touch touch buttons or touch screen.
3	Machine should have Acetate & Bicarbonate dialysis facility.
4	Machine should have Sequential/Isolation ultra filtration facility.
5.	It should have arterial, Venous & Transmembrane pressure monitoring facility.
5 a)	Arterial pressure Monitoring:-300mmHg to 280/300mmHg
5 b)	Venous pressure Monitoring:60mmHg to +500mmHg
5 c)	Transmembrane pressure Monitoring:60mmHg to+ 500mmHg
6	Treatment parameters should be displayed by trend curve and digital both.
7	Blood pump flow rate should be from 20ml/min to more or equal to 600 ml/min. Blood tubing pump segment should be operator changeable for use of different types of blood tubing sets (Blood pump tubing pump segment 4mm to 10 mm)
8	Machine should have volumetric ultrafiltration system.
9	Machine should have inbuilt on-line Dialysate fluid filter system for ultrapure dialysate delivery system for lot many treatments.
10	Machine should have In-line Bicarbonate mixing and solution preparation facility with sterile dry powder cartridge during dialysis.
11	Machines should have user friendly air bubble detector facility with level adjustment facility for venous chamber.
12	Machine should have optical sensor to check the presence of blood/saline in the extracorporeal blood circuit system.
13	Machine should have Heparin Infusion pump with rate 0 to 9.9/10 ml/min. and Bolus infusion up to 5 ml/min.
14	Machine should have blood leak sensor. Alarm will be activated for blood loss rate not greater than 0.5 ml/min at max, dialysate flow of 800 ml/min.
15	Machine should accept different concentrate formulation, different Dialyzer and blood tubing sets.
16	Machine should have variable Dialysate flow from 300 to 800 ml/min.
17	Machine should have dialysate temperature setting range 35°C to 39°C.
18	Ultrafiltration rate should be from 0 to 4.00 L/Hr.
19	Machine should have in house water filter assembly with cartridge filter.
20	Machine should have facility for priming and rinsing of dialyzer and blood lines.
21	Machine should have Hot rinsing and hot chemical disinfection facility (Temp. above 80 deg. Celsius) with recirculation system, with chemo/thermal cleansing and disinfection programs.
22	Machine should have ultrafiltration and sodium profiling facility.
23	Machine should have automatic battery backup of 20 minutes or more for complete Extracorporeal blood system during power failure.
24	Machine should have inbuilt online non-invasive patient blood pressure monitoring.(optional)
25	Machine should be upgradeable to future software developments and can be linked with patient data management system (optional)
26	Machine should be USFDA approved OR CE certified.
27	Power supply-230VAC,50 Hz
28	Should work on AC mains without batteries.
29	Operating & service manual with detail circuit diagram should be provided.
30	Machine should have real time clearance surveillance for urea & Kt/V to assess



	adequacy of dialysis. It should display real time Urea clearance, Plasma, Sodium, current Kt/V and time required to achieve Target Kt/V.
31	Training to MEC Engineer should be provision.
32	Should have strong service support backup. Give details of after sales service network.
33	Machine should have comprehensive warranty for 05 years.
34	Demonstration of the quoted model should be given with all above technical specifications.
35	Users list of quoted model with the addresses & contact Nos.to be provided.
36	Demonstration compulsory.
37	Tropicalization:
38a)	Operating room Temp.15°c up to 35°c
38b)	Storage room Temp 5°c up to 60°c
38c)	Relative humidity30% up to 75% non-condenser

